

# Rosemount Submersion Shield for the Rosemount 3107 and 3108




## About this guide

This guide provides instructions for fitting a Rosemount Submersion Shield (part number 03107-7003-0001) which is an optional accessory for the Rosemount 3107 Level and 3108 Flow transmitters.

It does not provide installation instructions for the Rosemount 3107 Level and 3108 Flow transmitters (or other optional accessories). Refer to the 3107/3108 reference manual (document no. 00809-0100-4840) for detailed instructions.

Product data sheets, reference manuals, and quick-start guides are available electronically on [www.emersonprocess.com](http://www.emersonprocess.com).

**Figure 1. Example application with a submersion shield fitted**

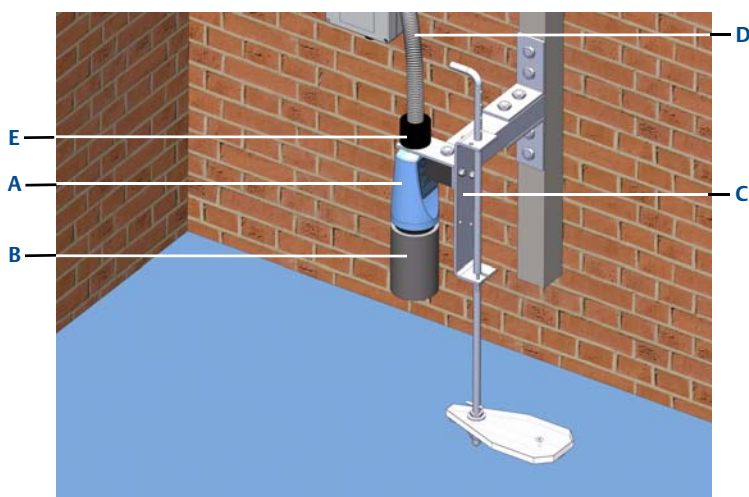

- A. Rosemount 3107 Level or 3108 Flow Transmitter
- B. Rosemount Submersion Shield (part number 03107-7003-0001)
- C. Rosemount Head Verification Device (part number 03107-7003-0005)
- D. Conduit (*not supplied*)
- E. Rosemount Conduit Adaptor Boss,
  - 1-in. BSP female to M20 x 1.5 female (part number 03107-7003-0003) or
  - 1-in. NPT female to 1½-in. NPT female (part number 03107-7003-0004)

## Rosemount 3107/3108 Submersion Shield


The Rosemount Submersion Shield (03107-7003-0001) is recommended for installations, e.g. wet wells, where a 3107/3108 transmitter may be at risk of being flooded.

It is easily fitted over the transducer cup, but requires the transmitter to be kept firmly vertical so that flood water causes an air pocket and keeps the transmitter face clear. The transmitter can then function normally when the flood water subsides.

Figure 1 on page 2 shows an example application with the submersion shield already fitted to a Rosemount 3107/3108 transmitter, which is then mounted on a Rosemount Head Verification Device.

---

**Figure 2. Features of the Rosemount Submersion Shield**

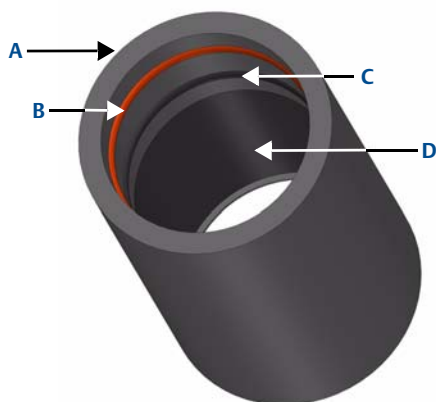

- A. PVC Submersion Shield (Medium Grey)
- B. Silicone O-ring (Red)
- C. Fluoroelastomer (FKM) O-ring (Dark Grey)
- D. Foam (PVC/NITRILE)

---

### WARNING

**Failure to follow these installation guidelines could result in death or serious injury**

- Make sure only qualified personnel perform the installation
- Use the equipment only as specified in this manual. Failure to do so may impair the protection provided by the equipment

**Electrical shock could cause death or serious injury**

- Make sure the main power to the transmitter is off and the lines to any other external power source are disconnected or not powered whilst installing the submersion shield
-

## Fitting the submersion shield

### Step 1: Check the transmitter mounting

The transmitter mounting must ensure that the transmitter is firmly kept in place, and ideally at 90 degrees to the liquid surface. This is essential for an air pocket to be formed at the base of the shield as flood water rises and passes it.

### Step 2: Lubricate both O-rings before fitting the shield


A suitable lubricant such as Dow Corning MS4 silicone grease may be used. If this is not available, a suitable water-based lubricant or liquid detergent may be used.

### Step 3: Fit the submersion shield

#### Follow this procedure:

1. Align the shield opening with the transducer cup, ensuring that the red O-ring is *above* the grey O-ring (Figure 3, left image).
2. Hold the transmitter and firmly push the shield upwards onto the transducer cup (Figure 3, middle image).
3. Continue pushing the shield upwards firmly until the red O-ring engages with the recess on the transducer cup (Figure 3, right image).

**Figure 3. Visual help for fitting the submersion shield**

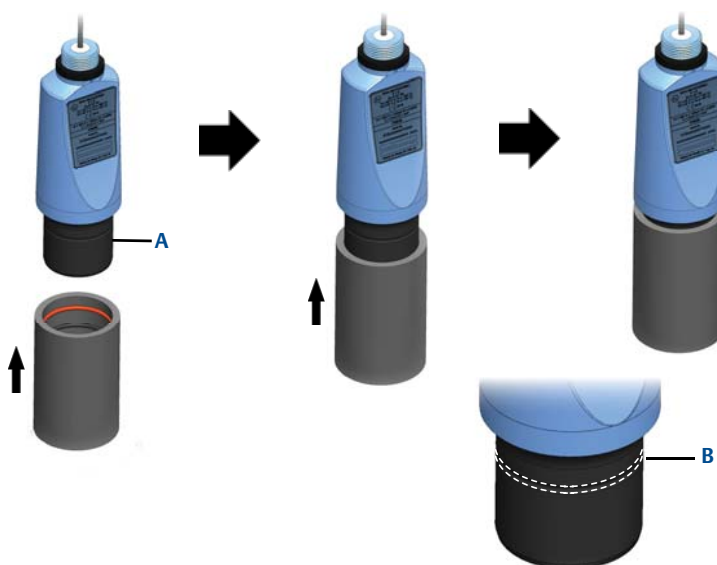

A. Transducer Cup

B. Recess on Transducer Cup


## Removing the submersion shield

This is only necessary for occasional cleaning or inspection in the event of contamination from flood water.

### Follow this procedure:

1. Holding the transmitter, pull the shield downwards firmly until the red O-ring is released from the recess on the transducer cup (Figure 4).
2. Continue to pull the shield downwards until it is free from the transducer cup.
3. Inspect the O-rings inside the shield for any signs of damage, and replace if necessary. Contact Rosemount for how to get replacements.

**Figure 4. Visual help for removing the submersion shield**

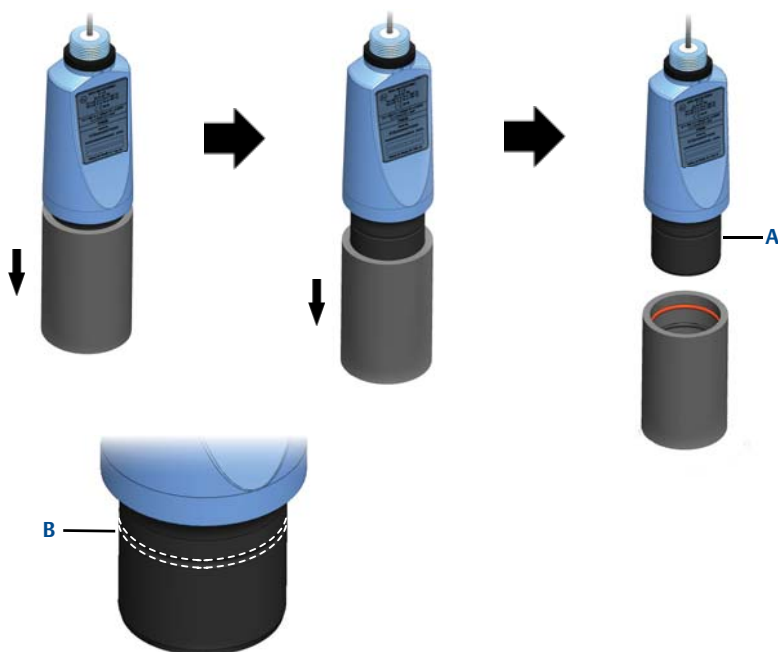

A. Transducer Cup

B. Recess on Transducer Cup





**Rosemount Inc.**  
8200 Market Boulevard  
Chanhassen, MN USA 55317  
T (US) (800) 999-9307  
T (Intl) (952) 906-8888  
F (952) 906-8889

**Emerson Process Management  
Asia Pacific Private Limited**  
1 Pandan Crescent  
Singapore 128461  
T (65) 6777 8211  
F (65) 6777 0947/65 6777 0743

**Emerson Process Management  
GmbH & Co. OHG**  
Argelsrieder Feld 3  
82234 Wessling Germany  
T 49 (8153) 9390, F 49 (8153) 939172

**Beijing Rosemount Far East  
Instrument Co., Limited**  
No. 6 North Street, Hepingli,  
Dong Cheng District  
Beijing 100013, China  
T (86) (10) 6428 2233  
F (86) (10) 6422 8586

© 2012 Rosemount Inc. All rights reserved. All marks property of owner.  
The Emerson logo is a trade mark and service mark of Emerson Electric Co  
Rosemount and the Rosemount logotype are registered trademarks of Rosemount Inc.